
























Responsible, Efficient, Reliable
PanSW Med Corp
www.panswmed.com













sales@panswmed.com
 pan-sw@hotmail.com
 Tel: 86-20-28961025
 Skype:panmedical; dianapansw





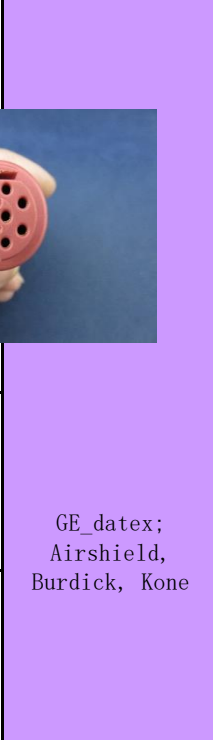

PANSW Part code	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10001A		Philips 78352A, M1165A, MerlinViridia 24, CMS 24 M3/M4, M1175A, M1350B, M1205A, M1350A, M1353A, 8030A, 8040A		Use with Abbott/Medex IBP transducer
IBP-10001B				Use with Utah IBP transducer
IBP-10001C				Use with Edward IBP transducer
IBP-10001D				Use with BD IBP transducer
IBP-10001E				Use with Argon IBP transducer
IBP-10001F				Use with B.Bruan IBP transducer









IBP-10001G				Use with dual connector Abbott/Medex
IBP-10001H				Use with Medex Logical
IBP-10001I				PVB transducer
IBP-101N4P				
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10002A		Siemens/Darger: SC6002XL, 7000, SC8000, SC9000XL		Use with Abbott/Medex IBP transducer
IBP-10002B				Use with Utah IBP transducer
IBP-10002C				Use with Edward IBP transducer
IBP-10002D				Use with BD IBP transducer












IBP-10002E				Use with Argon IBP transducer
IBP-10002F				Use with B. Bruan IBP transducer
IBP-10002H				Use with Medex Logical
IBP-10002I				PVB transducer
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10003A		Spacelabs monitors (for module 90496 requires adapter cable); original part number: 700-0028-00; Mindray: PM7000, 8000, 9000, 6201.		Use with Abbott/Medex IBP transducer
IBP-10003B				Use with Utah IBP transducer
IBP-10003C				Use with Edward IBP transducer
IBP-10003D				Use with BD IBP transducer
IBP-10003E				Use with Argon IBP transducer

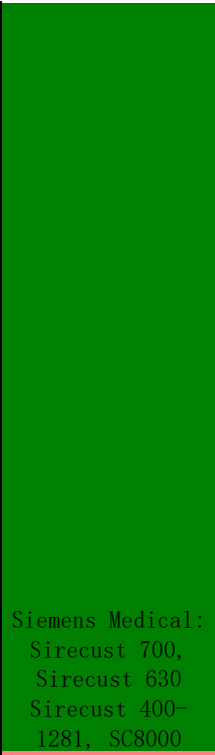



IBP-10003F				Use with B. Bruan IBP transducer
IBP-10003G				
IBP-10003H				
IBP-10003I				
IBP-10003SF				
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10004A	2021196-001/2021196-002			Use with Abbott/Medex IBP transducer
IBP-10004B	2016997-001/2016997-002			Use with Utah IBP transducer
IBP-10004C	2021197-001/2021197-002	GE Marquette; GE Solar, Dash, Eagle, Tram		Use with Edward IBP transducer
IBP-10004D	2016995-001/2016995-002			Use with BD IBP transducer


IBP-10004E				Use with Argon IBP transducer
IBP-10004F	GE part number: 22339301			Use with B. Brua IBP transducer
IBP-10004G				
IBP-10004H				
IBP-10004I	 		PVB transducer	
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10005A				Use with Abbott/Medex IBP transducer
IBP-10005B				Use with Utah IBP transducer
IBP-10005C				Use with Edward IBP transducer
IBP-10005D			GE_datex; Airshield, Burdick, Kone	





IBP-10005E				Use with Argon IBP transducer
IBP-10005F				Use with B.Brua IBP transducer
IBP-10005G				Use with USB connector
IBP-10005H				
IBP-10005I				PVB transducer
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10006A				Use with Abbott/Medex IBP transducer
IBP-10006B	K957 JP-960P			IBP Connection Cable for Biosensors Transducers, cable length: 3.5 m Applicable for Biosensors Transducers: series Biotrans & Series Accutrans For current products: all BSM/PVM-2703/TEC-8300
IBP-10006C	L901 JP-920P			IBP Connection Cable for Edwards Lifesciences Transducers, cable length: 3.5 m Applicable for Edwards Lifesciences Transducers: Series TruWave: PX-600P, PX-600F30, PX-600P, For current products: all BSM/PVM-2703/TEC-8300


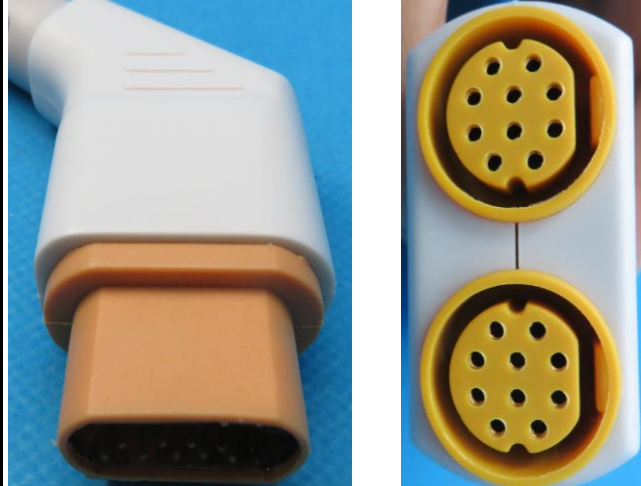
IBP-10006CS	L902 JP-921P	Nihon Kohden IPB cable; BSM-2300 Lifescope i/L; BSM-4100 Lifescope P; BSM-5100 Lifescope A; BSM-9510 Lifescope M; BSM-9800 Lifescope S;		IBP Connection Cable for Edwards Lifesciences Transducers, cable length: 1.5 m Applicable for Edwards Lifesciences Transducers: Series TruWave: PX-600P, PX-600F30, PX-600P, For current products: all BSM/PVM-2703/TEC-8300
IBP-10006D	K951 JP-900P			IBP Connection Cable for Becton Dickinson Transducers, cable length: 3.5 m Applicable for Becton Dickinson (Ohmeda) Transducers: all current models: series DTX/Plus & Series RT2000; older models: Series P23XL For current products: all BSM/PVM-2703/TEC-8300
IBP-10006E				Use with Argon IBP transducer
IBP-10006F				Use with B. Brua IBP transducer
IBP-10006I				PVB transducer
IBP-10007A				Use with Abbott/Medex IBP transducer





IBP-10007B				Use with Utah IBP transducer
IBP-10007C				Use with Edward IBP transducer
IBP-10007D				Use with BD IBP transducer
IBP-10007E				Use with Argon IBP transducer
IBP-10007F				Use with B. Brua IBP transducer
IBP-10007I				PVB transducer
IBP-10008A				Use with Abbott/Medex IBP transducer
IBP-10008B				Use with Utah IBP transducer
IBP-10008C				Use with Edward IBP transducer
IBP-10008D				Use with BD IBP transducer
IBP-10008E				Use with Argon IBP transducer


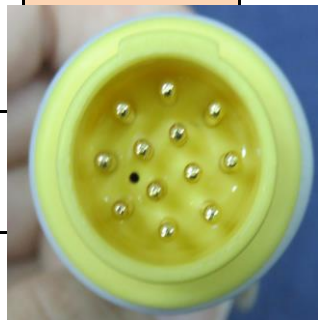

IBP-10008F				Use with B. Brua IBP transducer
IBP-10008I				PVB transducer
IBP-10009A		 Colin IBP cable		Use with Abbott/Medex IBP transducer
IBP-10009B				Use with Utah IBP transducer
IBP-10009C				Use with Edward IBP transducer
IBP-10009D				Use with BD IBP transducer
IBP-10009E				Use with Argon IBP transducer
IBP-10009F				Use with B. Brua IBP transducer
IBP-10009I				PVB transducer
IBP-10010A				Use with Abbott/Medex IBP transducer
IBP-10010B				Use with Utah IBP transducer
IBP-10010C				Use with Edward IBP transducer






IBP-10010D		CSI		Use with BD IBP transducer
IBP-10010E				Use with Argon IBP transducer
IBP-10010F				Use with B.Brui IBP transducer
IBP-10010I				PVB transducer
IBP-10011A		Mindray IBP cable		Use with Abbott/Medex IBP transducer
IBP-10011B				Use with Utah IBP transducer
IBP-10011C				Use with Edward IBP transducer
IBP-10011D				Use with BD IBP transducer
IBP-10011E				Use with Argon IBP transducer
IBP-10011F				Use with B.Brui IBP transducer
IBP-10011I				






IBP-10012A		 Fukuda IBP cable		Use with Abbott/Medex IBP transducer
IBP-10012B				Use with Utah IBP transducer
IBP-10012C				Use with Edward IBP transducer
IBP-10012D				Use with BD IBP transducer
IBP-10012E				Use with Argon IBP transducer
IBP-10012F				Use with B. Brua IBP transducer
IBP-10012I				
IBP-10013A		biolight IBP cable		Use with Abbott/Medex IBP transducer
IBP-10013B				Use with Utah IBP transducer
IBP-10013C				Use with Edward IBP transducer
IBP-10013D				Use with BD IBP transducer
IBP-10013E				Use with Argon IBP transducer
IBP-10013F				Use with B. Brua IBP transducer
IBP-10013I				






IBP-10014A		FUKUDA IBP cable		Use with Abbott/Medex IBP transducer
IBP-10014B				Use with Utah IBP transducer
IBP-10014C				Use with Edward IBP transducer
IBP-10014D				Use with BD IBP transducer
IBP-10014E				Use with Argon IBP transducer
IBP-10014F				Use with B.Brui IBP transducer
IBP-10014I				
IBP-10015A				drager dual connector adapter cable









IBP-10015B			small 7 pins connector * 2	drager dual connector adapter cable
IBP-10016A		 Nihon kohden IBP cable		Use with Abbott/Medex IBP transducer
IBP-10016B				Use with Utah IBP transducer
IBP-10016C				Use with Edward IBP transducer
IBP-10016D				Use with BD IBP transducer
IBP-10016E				Use with Argon IBP transducer
IBP-10016F				Use with B.Brue IBP transducer
IBP-10016I				
IBP-10017A		 datascope IBP cable		Use with Abbott/Medex IBP transducer
IBP-10017B				Use with Utah IBP transducer
IBP-10017C				Use with Edward IBP transducer
IBP-10017D				Use with BD IBP transducer

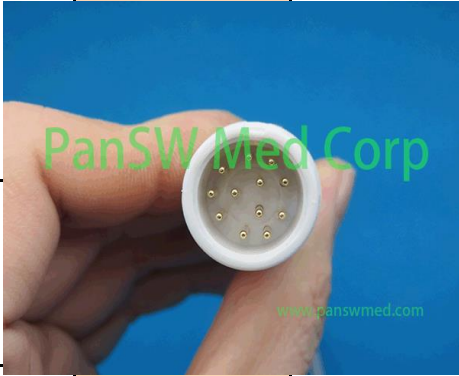





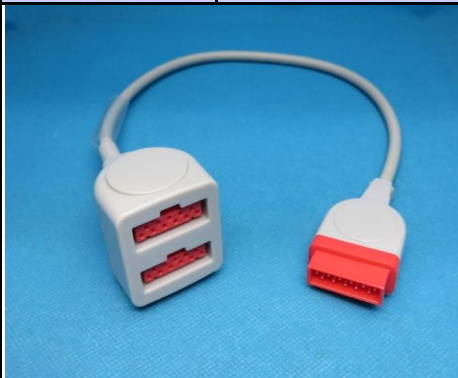

IBP-10017E				Use with Argon IBP transducer
IBP-10017F				Use with B. Brua IBP transducer
IBP-10017I				PVB
IBP-10018A				Use with Abbott/Medex IBP transducer
IBP-10018B				Use with Utah IBP transducer
IBP-10018C				Use with Edward IBP transducer
IBP-10018D		Kontron IBP cable Minimon 7131-7136, BC-KTN-AG BC-KTN-BB BC-KTN-BD BC-KTN-ED BC-KTN-MX BC-KTN-UT Fetalmon 2A, 2B Fetalogic 4000, Fetasonde 5, 5A, 5B K2000 Ballon Pump; KAAT II Module 10-7286, Supermon		Use with BD IBP transducer
IBP-10018E				Use with Argon IBP transducer
IBP-10018F				Use with B. Brua IBP transducer
IBP-10018I				
IBP-10019A		compatible MENNEN IBP CABLES; ENVOY, VITALOGIC		Use with Abbott/Medex IBP transducer
IBP-10019B				Use with Utah IBP transducer

IBP-10019C				Use with Edward IBP transducer
IBP-10019D				Use with BD IBP transducer
IBP-10019E				Use with Argon IBP transducer
IBP-10019F				Use with B. Brua IBP transducer
IBP-10019I				PVB
IBP-10020A		REDEL 6 PINS SINGLE NOTCH		Use with Abbott/Medex IBP transducer
IBP-10020B				Use with Utah IBP transducer
IBP-10020C				Use with Edward IBP transducer
IBP-10020D				Use with BD IBP transducer
IBP-10020E				Use with Argon IBP transducer
IBP-10020F				Use with B. Brua IBP transducer
IBP-10020I				PVB

IBP-10021A			Use with Abbott/Medex IBP transducer
IBP-10021B			Use with Utah IBP transducer
IBP-10021C			Use with Edward IBP transducer
IBP-10021D			Use with BD IBP transducer
IBP-10021E			Use with Argon IBP transducer
IBP-10021F			Use with B.Brue IBP transducer
IBP-10021I	<p>Compatible Spacelabs IBP cables; ultraview 90496 91496</p>	 	PVB
IBP-10022F			Use with B.Brue IBP transducer; dual heads (male & female)
IBP-10023A		<p>compatible GE Hollister IBP</p>	Use with Abbott/Medex IBP transducer
IBP-10023B			Use with Utah IBP transducer
IBP-10023C			Use with Edward IBP transducer

IBP-10023D		compatible IBP cables		Use with BD IBP transducer
IBP-10023E				Use with Argon IBP transducer
IBP-10023F				Use with B. Brua IBP transducer
IBP-10023I				PVB
IBP-10024A				Use with Abbott/Medex IBP transducer
IBP-10024B				Use with Utah IBP transducer
IBP-10024C				Use with Edward IBP transducer
IBP-10024D		compatible Comen C70 IBP cables		Use with BD IBP transducer
IBP-10024E				Use with Argon IBP transducer
IBP-10024F				Use with B. Brua IBP transducer

IBP-10024I	<div></div>			PVB
IBP-10025A	K952 JP-910P			compatible with Nihon Kohden IBP cables. IBP Adapter Cable for IBP Transducer Cables, BF type, cable length ; 0.3 m For current products: all BSM/PVM-2703/TEC- 8300
IBP-10026A	original part number: 2005772-001 30 cm/12 in			GE DUAL 2005772-001 30 cm/12 in 2103966-001
IBP-10027A	<div></div>			Use with Abbott/Medex IBP transducer
IBP-10027B				Use with Utah IBP transducer
IBP-10027C				Use with Edward IBP transducer
IBP-10027D				Use with BD IBP transducer
IBP-10027E				Use with Argon IBP transducer
IBP-10027F				Use with B.Brue IBP transducer

IBP-10027I	 		PVB	
IBP-10028A	2021196-003 Transpac-III/IV 3.6m/12ft 2021196-004 Transpac-III/IV	compatible GE dual heads IBP cables		Use with Abbott/Medex IBP transducer ICU Medical Transpac-IV®
IBP-10028B	2016997-003 3.6m/12ft 2016997-004 1.2m/4ft			Use with Utah IBP transducer Utah/Biotrans™
IBP-10028C	2021197-003 TruWave IP 3.6m/12ft 2021197-004 TruWave IP 1.2m/4 ft			Use with Edwards™ LS TruWave™ IBP transducer
IBP-10028D	2016995-003 3.6m/12 ft 2016995-004 1.2m/4 ft			Use with BD/Argon™ IBP transducer
IBP-10028E				Use with Argon IBP transducer
IBP-10027F				Use with B. Brua IBP transducer
IBP-10028I			PVB	
IBP-10029A		6 pins to GE adapter cable		Insinght

IBP-ORG		IBP transducer organizer	
---------	--	-----------------------------	--