



Responsible, Efficient, Reliable
PanSW Med Corp
www.panswmed.com

sales@panswmed.com
 pan-sw@hotmail.com
 Tel: 86-20-28961025
 Skype:panmedical; dianapansw

PANSW Part code	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10001A		Philips 78352A, M1165A, Merlin Viridia 24, CMS 24 M3/M4, M1175A, M1350B, M1205A, M1350A, M1353A, 8030A, 8040A		Use with Abbott/Medex IBP transducer
IBP-10001B				Use with Utah IBP transducer
IBP-10001C				Use with Edward IBP transducer
IBP-10001D				Use with BD IBP transducer
IBP-10001E				Use with Argon IBP transducer
IBP-10001F				Use with B.Bruan IBP transducer

IBP-10001G				Use with dual connector Abbott/Medex
IBP-10001H				Use with Medex Logical
IBP-10001I				PVB transducer
IBP-101N4P				
IBP-10001CD2				
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10002A				Use with Abbott/Medex IBP transducer

IBP-10002B		Siemens/Darger: SC6002XL, 7000, SC8000, SC9000XL		Use with Utah IBP transducer
IBP-10002C				Use with Edward IBP transducer
IBP-10002D	3375933			Use with BD IBP transducer
IBP-10002E				Use with Argon IBP transducer
IBP-10002F				Use with B.Bruan IBP transducer
IBP-10002H				Use with Medex Logical
IBP-10002I	 		PVB transducer	

IBP-10002CD2				
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10003A		Spacelabs monitors (for module 90496 requires adapter cable); original part number: 700-0028-00; Mindray: PM7000, 8000, 9000, 6201.		Use with Abbott/Medex IBP transducer
IBP-10003B				Use with Utah IBP transducer
IBP-10003C				Use with Edward IBP transducer
IBP-10003D				Use with BD IBP transducer
IBP-10003E				Use with Argon IBP transducer
IBP-10003F				Use with B.Bruan IBP transducer
IBP-10003G				

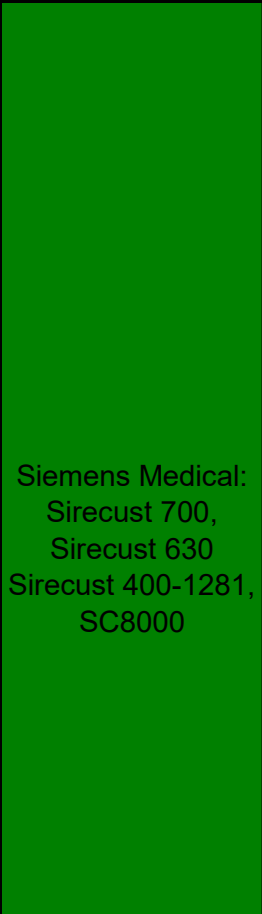
IBP-10003H				
IBP-10003I				
IBP-10003SF				
IBP-10003CD2				
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10004A	2021196-001/2021196-002			Use with Abbott/Medex IBP transducer

IBP-10004B	2016997-001/2016997-002	GE Marquette; GE Solar, Dash, Eagle, Tram		Use with Utah IBP transducer
IBP-10004C	2021197-001/2021197-002			Use with Edward IBP transducer
IBP-10004D	2016995-001/2016995-002			Use with BD IBP transducer
IBP-10004E				Use with Argon IBP transducer
IBP-10004F	GE part number: 22339301			Use with B.Brue IBP transducer
IBP-10004G				
IBP-10004H				

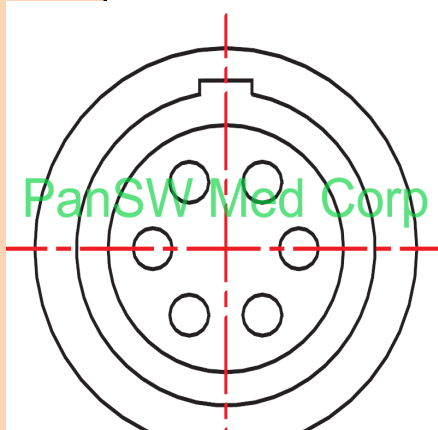
IBP-10004I			B transducer	
IBP-10004CD2				
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10005A		GE_datex; Airshield, Burdick, Kone		Use with Abbott/Medex IBP transducer
IBP-10005B				Use with Utah IBP transducer
IBP-10005C				Use with Edward IBP transducer
IBP-10005D				Use with BD IBP transducer
IBP-10005E				Use with Argon IBP transducer

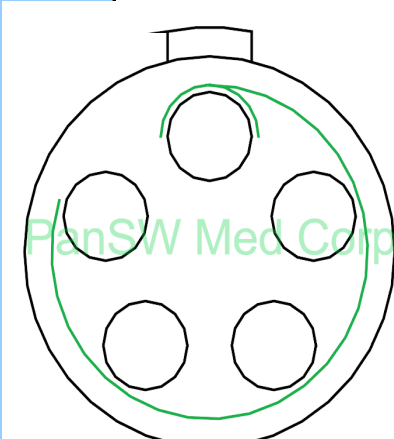
IBP-10005F				Use with B.Brua IBP transducer
IBP-10005G				Use with USB connector
IBP-10005H				
IBP-10005CD2				
IBP-10005I			 	PVB transducer
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10006A				Use with Abbott/Medex IBP transducer
IBP-10006B	K957 JP-960P			IBP Connection Cable for Biosensors Transducers, cable length: 3.5 m Applicable for Biosensors Transducers: series Biotrans & Series Accutrans For current products: all RSM/PVM-


IBP-10006C	L901 JP-920P	Nihon Kohden IBP cable; BSM-2300 Lifescope i/L; BSM-4100 Lifescope P; BSM-5100 Lifescope A; BSM-9510 Lifescope M; BSM-9800 Lifescope S; BSM-6701K		IBP Connection Cable for Edwards Lifesciences Transducers, cable length: 3.5 m Applicable for Edwards Lifesciences Transducers: Series TruWave: PX-600P, PX-600F30, PX-600P, For current products: all BSM/PVM-
IBP-10006CS	L902 JP-921P			IBP Connection Cable for Edwards Lifesciences Transducers, cable length: 1.5 m Applicable for Edwards Lifesciences Transducers: Series TruWave: PX-600P, PX-600F30, PX-600P, For current products: all BSM/PVM-2703/TEC-8300
IBP-10006D	K951 JP-900P			IBP Connection Cable for Becton Dickinson Transducers, cable length: 3.5 m Applicable for Becton Dickinson (Ohmeda) Transducers: all current models: series DTX/Plus & Series RT2000; older models: Series P23XL
IBP-10006E				Use with Argon IBP transducer

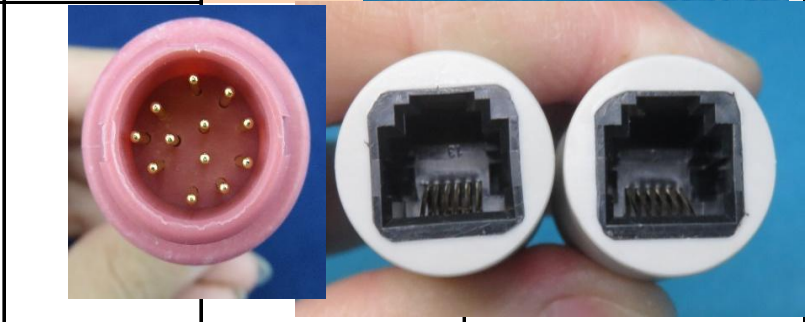
IBP-10006F			Use with B.Brua IBP transducer
IBP-10006I			PVB transducer
IBP-10006CD2			
IBP-10007A			Use with Abbott/Medex IBP transducer
IBP-10007B			Use with Utah IBP transducer
IBP-10007C			Use with Edward IBP transducer
IBP-10007D			Use with BD IBP transducer
IBP-10007E			Use with Argon IBP transducer

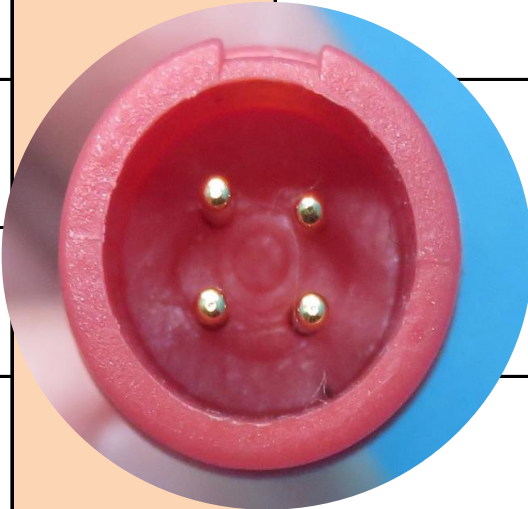
IBP-10007F			Use with B.Brua IBP transducer
IBP-10007I			PVB transducer
IBP-10007CD2			
IBP-10008A		datascope IBP cable System 80/82/83/84/90/90 T/95/98/97iabp850 /870/P2/P3/2000/2 000A/2001/2001A/ 2002/2002A/2200I/ 3000/Passport	Use with Abbott/Medex IBP transducer
IBP-10008B			Use with Utah IBP transducer
IBP-10008C			Use with Edward IBP transducer
IBP-10008D			Use with BD IBP transducer
IBP-10008E			Use with Argon IBP transducer

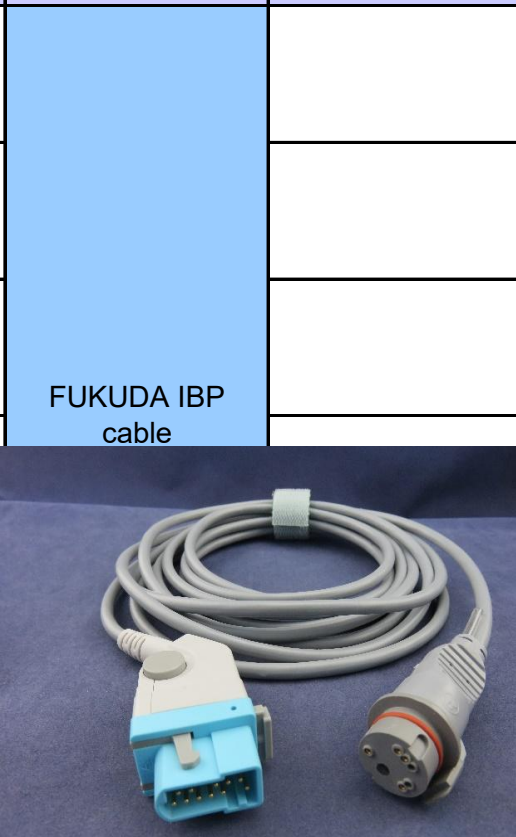
IBP-10008F				Use with B.Brua IBP transducer
IBP-10008I				PVB transducer
IBP-10008CD2				
IBP-10009A				Use with Abbott/Medex IBP transducer
IBP-10009B				Use with Utah IBP transducer
IBP-10009C				Use with Edward IBP transducer
IBP-10009D			Colin IBP cable	Use with BD IBP transducer
IBP-10009E				Use with Argon IBP transducer
IBP-10009F				Use with B.Brua IBP transducer

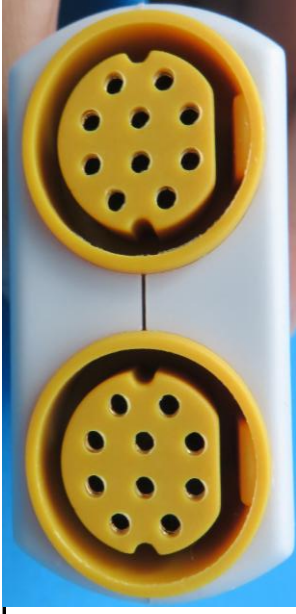
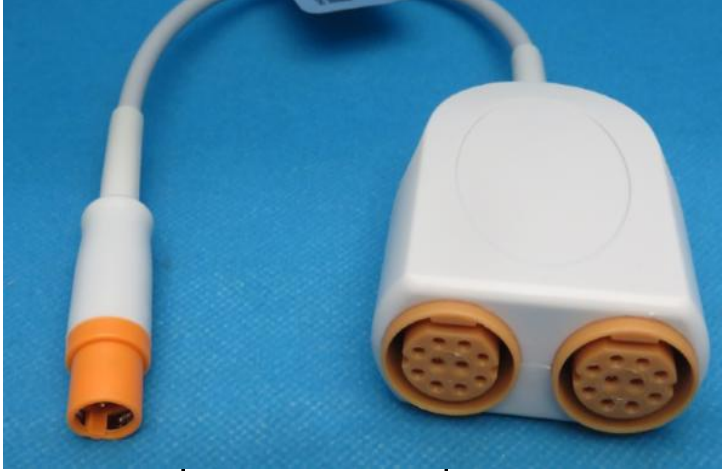
IBP-10009I			PVB transducer
IBP-10009CD2			
IBP-10010A			Use with Abbott/Medex IBP transducer
IBP-10010B			Use with Utah IBP transducer
IBP-10010C			Use with Edward IBP transducer
IBP-10010D			Use with BD IBP transducer
IBP-10010E			Use with Argon IBP transducer
IBP-10010F		CSI IBP cable Scholar 8100 Scholar 2200 	Use with B.Brue IBP transducer

IBP-10010I				PVB transducer
IBP-10010CD2				
IBP-10011A		 Mindray IBP cable		Use with Abbott/Medex IBP transducer
IBP-10011B				Use with Utah IBP transducer
IBP-10011C				Use with Edward IBP transducer
IBP-10011D				Use with BD IBP transducer
IBP-10011E				Use with Argon IBP transducer
IBP-10011F				Use with B.Bruea IBP transducer

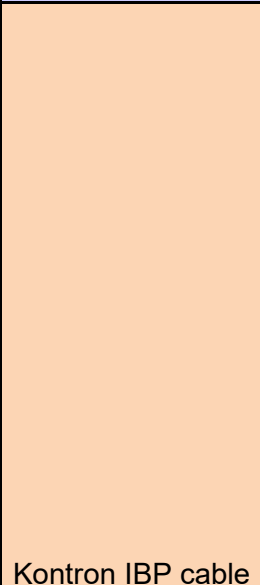
IBP-10011I				
IBP-10011A2				
IBP-10011CD2				
IBP-10012A		 Fukuda IBP cable		Use with Abbott/Medex IBP transducer
IBP-10012B				Use with Utah IBP transducer
IBP-10012C				Use with Edward IBP transducer
IBP-10012D				Use with BD IBP transducer
IBP-10012E				Use with Argon IBP transducer
IBP-10012F				Use with B.Brue IBP transducer

IBP-10012I			
IBP-10012CD2			
IBP-10013A		biolight IBP cable 	Use with Abbott/Medex IBP transducer
IBP-10013B			Use with Utah IBP transducer
IBP-10013C			Use with Edward IBP transducer
IBP-10013D			Use with BD IBP transducer
IBP-10013E			Use with Argon IBP transducer
IBP-10013F			Use with B.Brua IBP transducer
IBP-10013I			

IBP-10013CD2				
IBP-10014A		 FUKUDA IBP cable		Use with Abbott/Medex IBP transducer
IBP-10014B				Use with Utah IBP transducer
IBP-10014C				Use with Edward IBP transducer
IBP-10014D				Use with BD IBP transducer
IBP-10014E				Use with Argon IBP transducer
IBP-10014F				Use with B.Brui IBP transducer
IBP-10014I				
IBP-10014CD2				

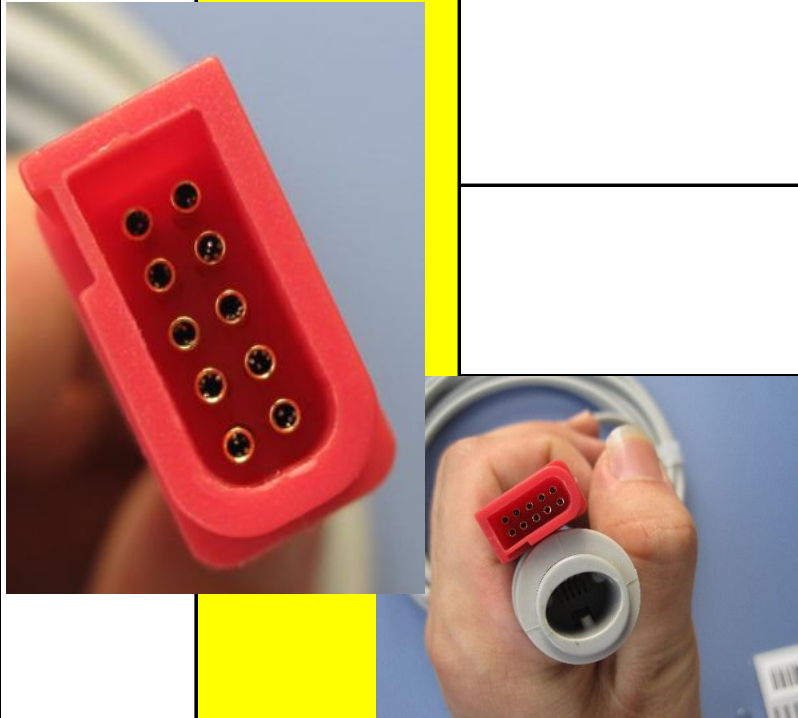
IBP-10015A				drager dual connector adapter cable
IBP-10015B		small 7 pins connector * 2		drager dual connector adapter cable
IBP-10015C				
IBP-10016A		Nihon kohden IBP cable Lifescope 6/9/12/14 AP-311P 600-501400		Use with Abbott/Medex IBP transducer

IBP-10016B		-800pa BSM2100 8500A OEC 3200 8120A OMP- 3221E N8203 Mercury 9510K		Use with Utah IBP transducer
IBP-10016C				Use with Edward IBP transducer
IBP-10016D				Use with BD IBP transducer
IBP-10016E				Use with Argon IBP transducer
IBP-10016F				Use with B.Brue IBP transducer
IBP-10016I				
IBP-10016CD2				
IBP-10017A		datascope IBP cable		Use with Abbott/Medex IBP transducer
IBP-10017B				Use with Utah IBP transducer
IBP-10017C				Use with Edward IBP transducer

IBP-10017D				Use with BD IBP transducer
IBP-10017E				Use with Argon IBP transducer
IBP-10017F				Use with B.Brue IBP transducer
IBP-10017I				PVB
IBP-10017CD2				
IBP-10018A				Use with Abbott/Medex IBP transducer
IBP-10018B				Use with Utah IBP transducer
IBP-10018C				Use with Edward IBP transducer
IBP-10018D				Use with BD IBP transducer

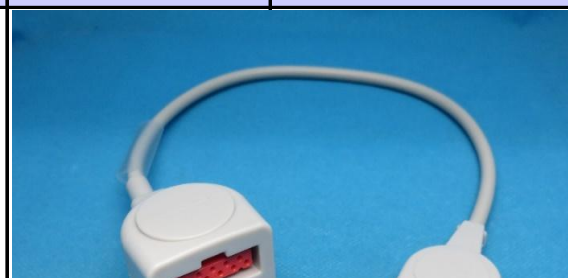
IBP-10018E		Minimon 7131-7136, Fetalmon 2A,2B Fetalogic 4000, Fetasonde 5,5A,5B K2000 Ballon Pump; KAAT II Module 10-7286, Supermon		Use with Argon IBP transducer
IBP-10018F				Use with B.Brua IBP transducer
IBP-10018I				
IBP-10018CD2				
IBP-10019A		compatible MENNEN IBP CABLES; ENVOY, VITALOGIC		Use with Abbott/Medex IBP transducer
IBP-10019B				Use with Utah IBP transducer
IBP-10019C				Use with Edward IBP transducer
IBP-10019D				Use with BD IBP transducer
IBP-10019E				Use with Argon IBP transducer

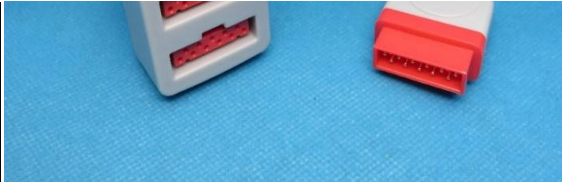
IBP-10019F			Use with B.Brue IBP transducer
IBP-10019I			PVB
IBP-10019CD2			
IBP-10020A		MOST CARE UP REDEL 6 PINS SINGLE NOTCH	Use with Abbott/Medex IBP transducer
IBP-10020B			Use with Utah IBP transducer
IBP-10020C			Use with Edward IBP transducer
IBP-10020D			Use with BD IBP transducer
IBP-10020E			Use with Argon IBP transducer
IBP-10020F			Use with B.Brue IBP transducer

IBP-10020I			PVB
IBP-10020CD2			
IBP-10021A			Use with Abbott/Medex IBP transducer
IBP-10021B			Use with Utah IBP transducer
IBP-10021C			Use with Edward IBP transducer
IBP-10021D			Use with BD IBP transducer
IBP-10021E			Use with Argon IBP transducer
IBP-10021F			Use with B.Brua IBP transducer
Compatible Spacelabs IBP cables; ultraview 90496 91496			

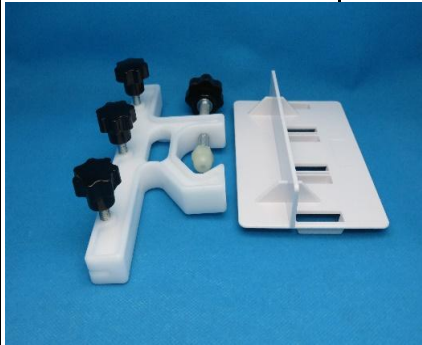
IBP-10021I				PVB
IBP-10021CD2				
IBP-10022F				Use with B.Brua IBP transducer; dual heads(male & female)
IBP-10023A		compatible GE Hellige IBP cables		Use with Abbott/Medex IBP transducer
IBP-10023B				Use with Utah IBP transducer
IBP-10023C				Use with Edward IBP transducer
IBP-10023D				Use with BD IBP transducer
				Use with Argon IBP transducer

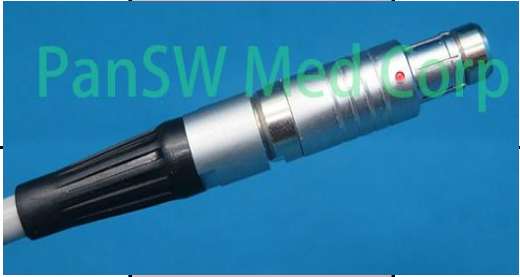
				Use with B.Brua IBP transducer
				PVB
IBP-10023CD2				
IBP-10024A				Use with Abbott/Medex IBP transducer
IBP-10024B				Use with Utah IBP transducer
IBP-10024C		compatible Comen C70 IBP cables		Use with Edward IBP transducer
IBP-10024D				Use with BD IBP transducer

IBP-10024E				Use with Argon IBP transducer
IBP-10024F				Use with B.Brua IBP transducer
IBP-10024I				PVB
IBP-10024CD2				
IBP-10025A	K952 JP-910P			compatible with Nihon Kohden IBP cables. IBP Adapter Cable for IBP Transducer Cables, BF type, cable length ; 0.3 m For current products: all BSM/PVM-2703/TEC-8300
IBP-10026A	original part number: 2005772-001			GE DUAL 2005772-001 30 cm/12 in 2103966-001

	30 cm/12 in		
IBP-10027A			Use with Abbott/Medex IBP transducer
IBP-10027B			Use with Utah IBP transducer
IBP-10027C			Use with Edward IBP transducer
IBP-10027D			Use with BD IBP transducer
IBP-10027E			Use with Argon IBP transducer
IBP-10027F			Use with B.Brua IBP transducer
IBP-10027I			PVB

IBP-10027CD2				
IBP-10028A	2021196-003 Transpac-III/IV 3.6m/12ft 2021196-004 Transpac-III/IV	compatible GE dual heads IBP cables		Use with Abbott/Medex IBP transducer ICU Medical Transpac-IV®
IBP-10028B	2016997-003 3.6m/12ft 2016997-004 1.2m/4ft			Use with Utah IBP transducer Utah/Biotrans™
IBP-10028C	2021197-003 TruWave IP 3.6m/12ft 2021197-004 TruWave IP 1.2m/4 ft			Use with Edwards™ LS TruWave™ IBP transducer
IBP-10028D	2016995-003 3.6m/12 ft 2016995-004 1.2m/4 ft			Use with BD/Argon™ IBP transducer
IBP-10028E				Use with Argon IBP transducer
IBP-10028F				Use with B.Brua IBP transducer

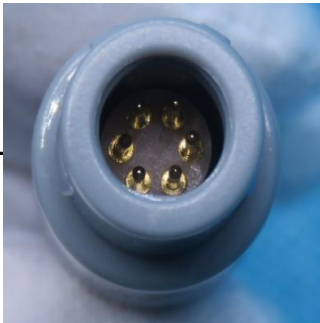
IBP-10028I				PVB
IBP-10028CD2				
IBP-10029A		6 pins to GE adapter cable		Insinght
IBP-ORG		IBP transducer organizer		
IBP-10030		Philips IBP cable adapter dual heads to Philips		
IBP-10031A				Use with Abbott/Medex IBP transducer

IBP-10031B			Use with Utah IBP transducer
IBP-10031C			Use with Edward IBP transducer
IBP-10031D			Use with BD IBP transducer
IBP-10031E		compatible ECMO-IBP cables	Use with Argon IBP transducer
IBP-10031F			Use with B.Brua IBP transducer
IBP-10031I	 		PVB
IBP-1003CD2I			

IBP-10032A			Spacelabs Healthcare mdoelo : XPREZZON
IBP-10033A		compatible GE Corometrics	Use with Abbott/Medex IBP transducer
IBP-10033B			Use with Utah IBP transducer
IBP-10033C			Use with Edward IBP transducer
IBP-10033D			Use with BD IBP transducer
IBP-10033E			Use with Argon IBP transducer

IBP-10033F				Use with B.Brua IBP transducer
IBP-10033I				PVB
IBP-10033CD2				
IBP-10034A				Use with Abbott/Medex IBP transducer
IBP-10034B				Use with Utah IBP transducer
IBP-10034C				Use with Edward IBP transducer
IBP-10034D				Use with BD IBP transducer
IBP-10034E		compatible Comen old model IBP cables		Use with Argon IBP transducer

IBP-10034F		cables		Use with B.Brua IBP transducer
IBP-10034I				PVB
IBP-10034CD2				
IBP-10035A				Use with Abbott/Medex IBP transducer
IBP-10035B				Use with Utah IBP transducer
IBP-10035C				Use with Edward IBP transducer
IBP-10035D				Use with BD IBP transducer
IBP-10035E		compatible Contec new model IBP cables		Use with Argon IBP transducer

IBP-10035F				Use with B.Brua IBP transducer
IBP-10035I				PVB
IBP-10035CD2				
IBP-10036		compatible Biolight IBP adapter		
IBP-10037A		compatible Nihon Kohden SVM 7500 7600 IBP cables		Use with Abbott/Medex IBP transducer
IBP-10037B				Use with Utah IBP transducer
IBP-10037C				Use with Edward IBP transducer

IBP-10037D					Use with BD IBP transducer
IBP-10037E					Use with Argon IBP transducer
IBP-10037F					Use with B.Brua IBP transducer